Vol. 29
Contents

2005

Contents of Volume 29 (2005)

NUMBER 1 JANUARY – FEBRUARY 2005

A micro creeping robot for colonoscopy based on the earthworm
J. Zuo, G. Yan and Z. Gao 1

Real time measurement of RR intervals using a digital signal processor
A. C. Buttfield and M. P. Bolton 8

Biomechanics in augmentation rhinoplasty
J. Yang, X. Wang, Y. Zeng and W. Wu 14

A new method to detect systemic inflammatory response syndrome by continuous monitoring system: an experimental study in rats
T. Matsui, T. Ishizuka, M. Ishihara, M. Suzuki, A. Kurita and M. Kikuchi 18

Non-invasive glycaemia blood measurements by electromagnetic sensor: Study in static and dynamic blood circulation
M. Gourzi, A. Rouane, R. Guelaz, M. S. Alavi, M. B. McHugh, M. Nadi and P. Roth 22

Low cost CCD camera protection against neutron radiation damage
J. G. M. Kok 27

A new strategy for easy volume conductor modelling in magnetocardiography
W. Tedeschi, H.-P. Müller, B. Schless, O. Grebe, V. Hombach, U. P. C. Neves, O. Baffa and S. N. Ern 33

How information technologies have improved both productivity and quality of health care
S. Tao Jiang 38

A new approach for detection of leg movement using segmental electrical impedance changes
C.-G. Song, J.-H. Seo, K.-S. Kim, D.-Y. Youn and D. Won Kim 42

MHRA Publications 47

News and Product Update 49

Calendar 52

NUMBER 2 MARCH–APRIL 2005

Automatic segmentation of medical images using image registration: diagnostic and simulation applications
D. C. Barber and D. R. Hose 53

A fuzzy logic based closed-loop control system for blood glucose level regulation in diabetics
M. S. Ibbini and M. A. Masadeh 64

A kinetic model for simulation of blood coagulation and inhibition in the intrinsic path
Y. H. Qiao, J. L. Liu and Y. J. Zeng 70

A thermodynamic model to predict the thermal response of living beings during pneumoperitoneum procedures
J. V. C. Vargas, D. Vlassov, D. Colman and M. L. Brioschi 75

Stimulated muscle force assessment of the sternocleidomastoid muscle in humans
J. Hong, J. H. Falkenberg and P. A. Iaizzo 82

A quantitative gait assessment method based on energy exchange analysis during walking: a normal gait study
F. Gider, Z. Matjaččić and T. Bajd 90

An improved windowing technique for heart rate variability power spectrum estimation
D. Singh, K. Vinod, S. C. Saxena and K. K. Deepak 95

Book Review 102

MHRA Publications 103

Calendar 105

NUMBER 3 MAY–JUNE 2005

Device Evaluation Service for UK Medical Equipment

Editorial 107

Medical device evaluation in the United Kingdom: past, present and future
D. C. Crawford 108

Oscillometric blood pressure devices and simulators: measurements of repeatability and differences between models
A. J. Sims, C. A. Reay, D. R. Bousfield, J. A. Menes and A. Murray 112

Evaluation of alternative computer input devices used by people with disabilities
G. Turpin, J. Armstrong, P. Frost, B. Fine, C. D. Ward and L. L. Pinnington 119

Very small air bubbles (10–70 μl) cause clinically significant variability in syringe pump fluid delivery
C. Davey and T. Stather-Dunn 130

Evaluation of text telephones designed for people with impaired hearing or speech
J. Spicer, R. Schmidt, C. D. Ward and L. L. Pinnington 137

MHRA Publications 145

News & Product Update 147

Calendar 150

NUMBER 4 JULY–AUGUST 2005

The Middlesex University rehabilitation robot 151
B. Parsons, A. White, S. Prior and P. Warner

Assessment of patient support surfaces: principle, practice and limitations 163
S. Rithalia

Unipolar cardiac pacemakers in electromagnetic fields of high voltage overhead lines 170
A. Scholten, S. Joosten and J. Silny

A new approach to detect QRS complexes based on a histogram and genetic algorithm 176
C. Tu, Y. Zeng and X. Yang

Fabrication and analysis of plastic hypodermic needles 181
H. Kim and J. S. Colton

Computational simulation of biomechanics in e-PTFE and venous Miller's cuffs: Implications for intimal hyperplasia 187
X.-M. Li and S. E. Rittgers

MHRA and DES Publications Update 197

News and Product Update 199

Calendar 202

NUMBER 5 SEPTEMBER – OCTOBER 2005

Surface myoelectric signal classification for prostheses control
Y. Al-Assaf and H. Al-Nashash 203

Homomorphic wavelet thresholding technique for denoising medical ultrasound images
S. Gupta, R. C. Chauhan and S. C. Saxena 208

Electric current perception of the general population including children and the elderly
N. Leitgeb, J. Schroettner and R. Cech 215

Frequency-plane analysis of normal and pathological ECG signals for disease identification
S. Mitra, S. Mitra and B. B. Chaudhuri 219

Continuous and online analysis of heart rate variability
H. L. Chan, W. S. Chou, S. W. Chen, S. C. Fang, C. S. Liou and Y. S. Hwang 227

A novel permanent maglev rotary LVAD with passive magnetic bearings
K. X. Qian, H. Y. Yuan, P. Zeng and W. M. Ru 235

Subtraction procedure for powerline interference removing from ECG: improvement for non-multiple sampling
G. Mihov, Iv. Dotsinsky and Ts. Georgieva 238

Technical Note: Performance evaluation of stereo endoscopic imaging system incorporating TFT-LCD
C.-G. Song and S.-K. Park 244

MHRA and DES Publications Update 251

News and Product Update 253

Calendar 256

NUMBER 6 NOVEMBER – DECEMBER 2005

A perspective on medical infrared imaging
L. J. Jiang, E. Y. K. Ng, A. C. B. Yeo, S. Wu, F. Pan, W. Y. Yau, J. H. Chen and Y. Yang 257

Electrical potentials derived from articular cartilage: the significance of polarization potentials
B. Schmidt-Rohlfing, K. Gavenis and J. Silny 268

Micromachined oxygen gas sensors for microscopic energy consumption measurement systems
C.-C. Wu, G.-B. Lee, M.-H. Chen and C.-H. Luo 278

An algorithm for synchronization of in vivo electroporation with ECG
B. Mali, T. Jarm, F. Jager and D. Miklavčič 288

Performance improvement of the SPIHT coder based on statistics of medical ultrasound images in the wavelet domain
L. Kaur, R. C. Chauhan and S. C. Saxena 297

World-first implantable aortic valvo-pump (IAVP) with sufficient haemodynamic capacity
K. X. Qian, D. F. Wang, S. Topaz, P. Zeng, W. M. Ru, H. Y. Yuan and J. B. Zwischenberg 302

MHRA and CEP Publications Update 305

News and Product Update 308
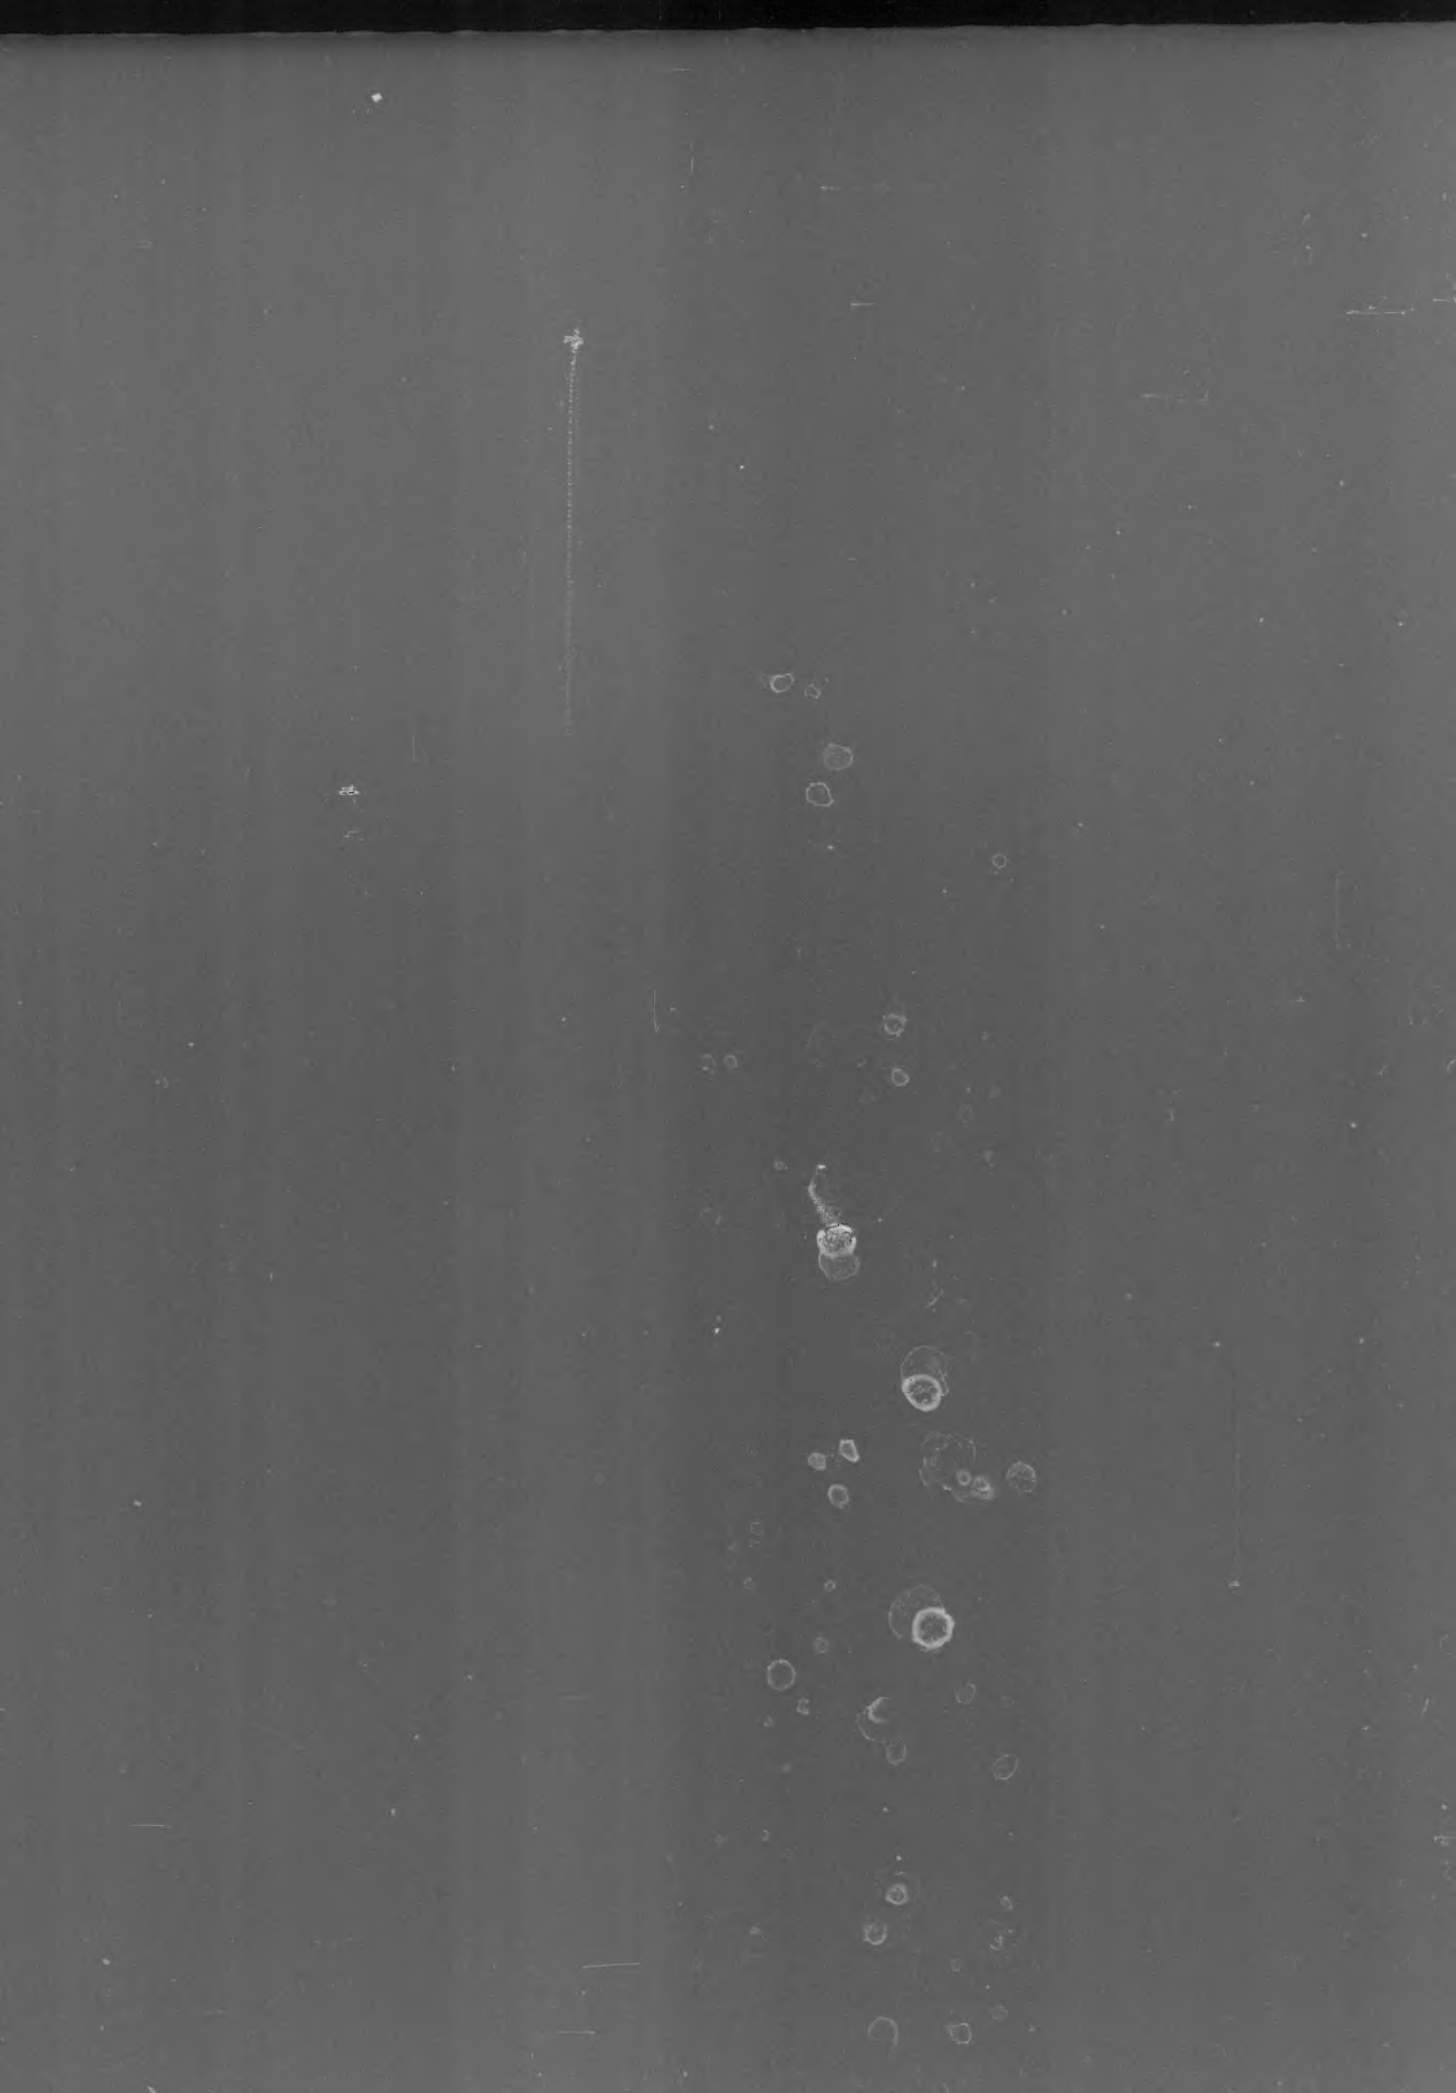
Calendar 311